

**CHINA GUANGZHOU  
KANGLING MEDICAL**

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

# **DISPOSABLE PROTECTIVE MASK**



# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## ABOUT KANGLING MEDICAL

Guangzhou Kangling Medical Supplies Co., Ltd. covers an area of 10,000 square meters and a construction area of more than 58,000 square meters. It is the first production base of epidemic prevention and protective materials in China with the whole industry chain. It mainly produces disposable medical masks, medical surgical masks, medical protective masks, disposable children's masks, disposable protective masks, FFP2, FFP3 protective masks, KN95 protective masks. Masks, melt-blown cloth, etc.

Kangling Medical has 1,500 employees and a group of professional R&D teams that combine theory and practice. Innovative design, marketing, service, and network services are integrated. Kangling provides you with the best quality products at good prices. Serve. Kangling Medical builds an ecosystem of medical protection products, creates an honest, transparent and win-win supply chain system, and becomes a leader in the medical protection industry.

Kangling is responsible for every healthy breath!

Kangling uses quality to build a solid wall of epidemic prevention for the world!



# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH



## QUALITY CONTROL

- ISO 9001 Quality Management System Certification
- ISO 13485 Medical Device Quality Management System
- FDA registration certificate
- TUV test report
- SGS test report

# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## NY TIMES SQUARE

The world sees Kangling! Kangling shines in Times Square, New York, USA!




# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## MATERIAL COMPOSITION OF PROTECTIVE MASKS

Disposable Protective Mask Has A Multilayer Design. It Is Crafted From Non-woven Filtering Materials, embedded With Electrostatic Charged Microfibers.

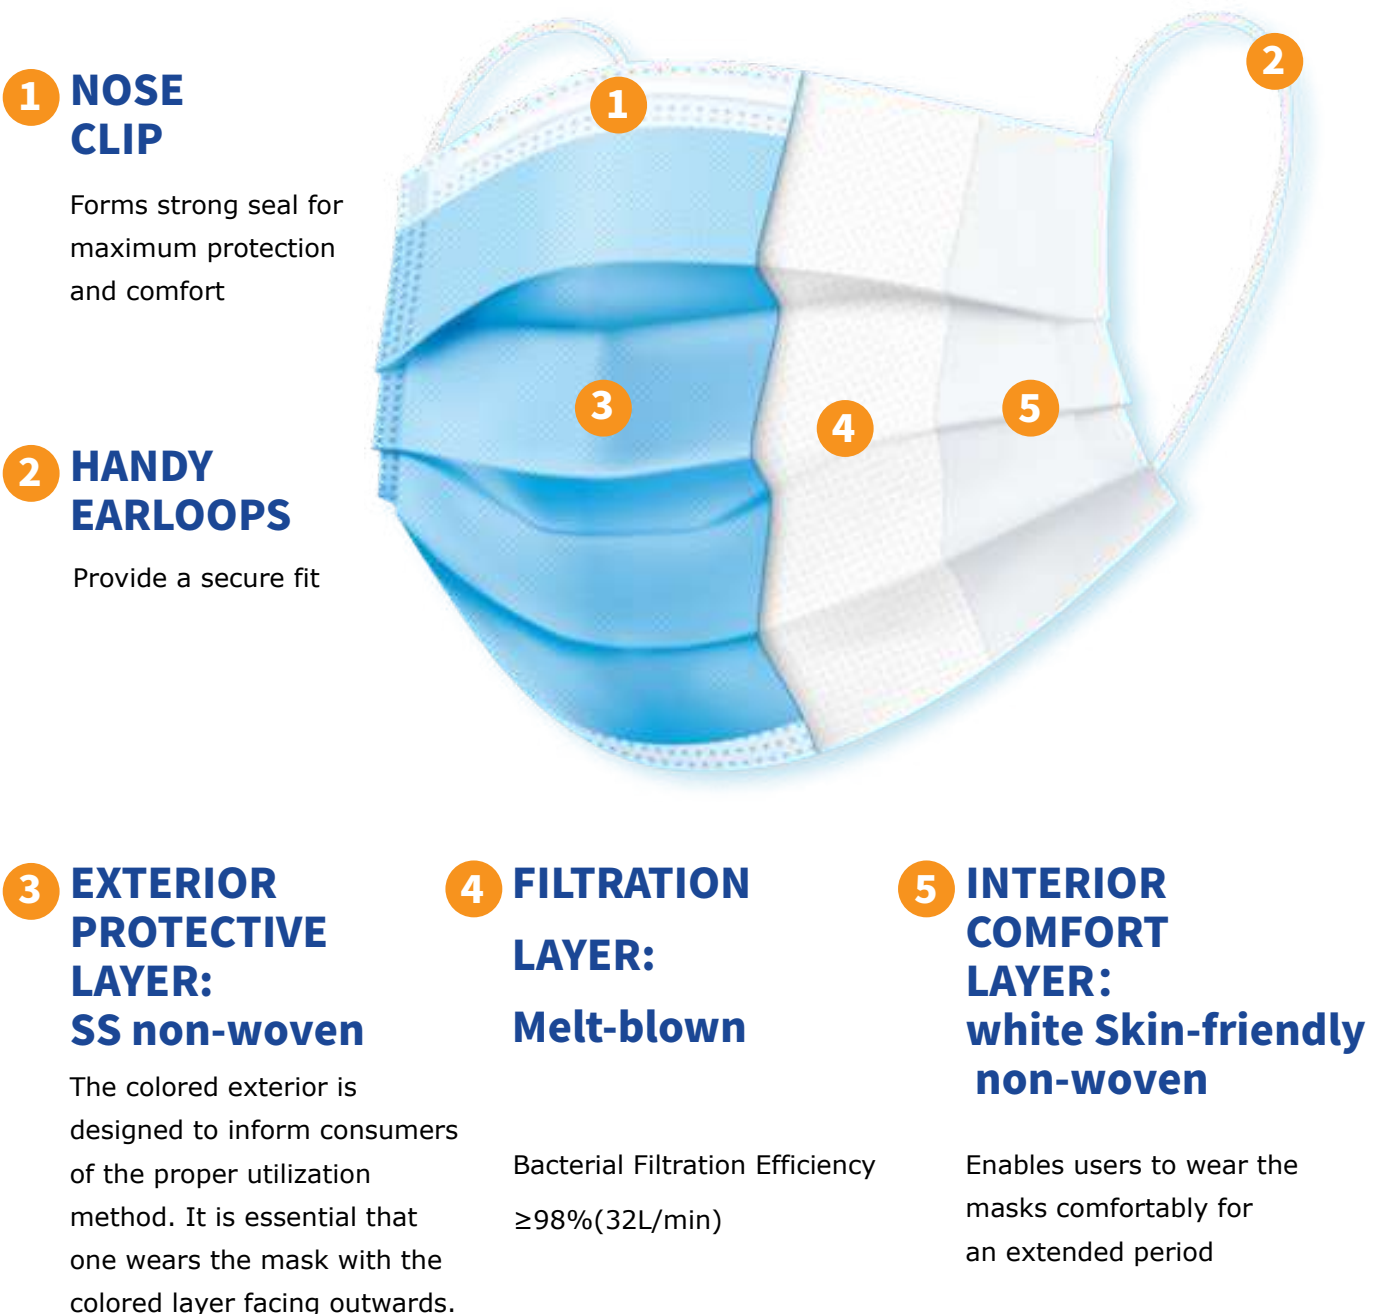

## TECHNICAL DATA SHEET

The colors of the masks are:  
blue、 pink、 black

### [Range of Application]

Provide protection to the relevant personnel against inhaling airborne particles through respiratory tract.



Product Name	DISPOSABLE PROTECTIVE MASK
Product Dimension	175x95mm
Product	Non-medical
Shelf Life	2 years
Material	25g SS non-woven fabric 25g melt blown fabric 25g white Skin-friendly non-woven fabric
Performance	Strap: 3.0mm flat or round ear Strap
	Bacterial Filtration Efficiency (BFE) ≥98%(32L/min)
	Inhalation Exhalation Resistance ≤49Pa/cm <sup>2</sup>
	Ear loop pull test 10N
	Nose piece: 10.5-11cm


# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## PACKAGE DESIGNS (BLUE MASK)

### Exterior Design

- Size: 180\*100\*70mm
- Gross weight: 190g




**50**  
Units



### Carton Design

- 40 boxes/carton
- Size: 520\*380\*300mm
- Gross weight: 8.4kg



**2000**  
Units



### Storage And Disposal



# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## PACKAGING FLOW CHART (BLUE MASK)

<p style="text-align: center;">1</p> 	<p style="text-align: center;">2</p> 	<p style="text-align: center;">3</p> 
<p>The inner buckle of the ear rope is neat, and the nose bridge strips are staggered and stacked up and down (25 pieces each)</p>	<p>Put it in a PE bag and seal it</p>	<p>Put in a color box and put the certificate of conformity</p>
<p style="text-align: center;">4</p> 	<p style="text-align: center;">5</p> 	<p style="text-align: center;">6</p> 
<p>Put the seal on the designated location</p>	<p>Seal the top of the carton with sealing glue</p>	<p>Put it in a moisture-proof bag and flatten the bottom layer</p>
<p style="text-align: center;">7</p> 	<p style="text-align: center;">8</p> 	<p style="text-align: center;">9</p> 
<p>The color box also needs to be turned over and put into a moisture-proof bag. The side is white. The outer box is affixed with a certificate of conformity.</p>	<p>Finally, flatten the moisture-proof bag, and insert the excess film into the side</p>	<p>Seal the box, turn it over and place it upwards and paste the certificate on the designated position</p>



# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## PACKAGE DESIGNS (PINK MASK)

### Exterior Design

- Size: 180\*100\*70mm
- Gross weight: 190g



**50**  
Units



### Carton Design

- 40 boxes/carton
- Size: 520\*380\*300mm
- Gross weight: 8.4kg



**2000**  
Units



### Storage And Disposal



# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## PACKAGING FLOW CHART (PINK MASK)

1	2	3
		
<p>The inner buckle of the ear rope is neat, and the nose bridge strips are staggered and stacked up and down (25 pieces each)</p>	<p>Put it in a PE bag and seal it</p>	<p>Put in a color box and put the certificate of conformity</p>
4	5	6
		
<p>Put the seal on the designated location</p>	<p>Seal the top of the carton with sealing glue</p>	<p>Put it in a moisture-proof bag and flatten the bottom layer</p>
7	8	9
		
<p>The color box also needs to be turned over and put into a moisture-proof bag. The side is white. The outer box is affixed with a certificate of conformity.</p>	<p>Finally, flatten the moisture-proof bag, and insert the excess film into the side</p>	<p>Seal the box, turn it over and place it upwards and paste the certificate on the designated position</p>


# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## PACKAGE DESIGNS (BLACK MASK)

### Exterior Design

- Size: 180\*100\*70mm
- Gross weight: 190g




**50**  
Units



### Carton Design

- 40 boxes/carton
- Size: 520\*380\*300mm
- Gross weight: 8.4kg



**2000**  
Units



### Storage And Disposal



# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## QUALITY CONTROL

- ISO 9001 Certification





# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## QUALITY CONTROL

- FDA Certificate

The screenshot shows the FDA's public database for Establishment Registration & Device Listing. The search results are filtered by 'Owner Operator Name' to 'Guangzhou kangling', showing 2 results. The first result is for 'GUANGZHOU KANGLING BIOTECHNOLOGY CO., LTD' in China, with no registration number listed and a current registration year of 2022. The second result is for 'GUANGZHOU KANGLING MEDICAL SUPPLIES COMPANY LIMITED' in China, with registration number 3017125486 and a current registration year of 2021. Both entries list various medical devices such as non-surgical isolation gowns, latex gloves, and respirators.

U.S. FOOD & DRUG ADMINISTRATION

Follow FDA | En Español

SEARCH

Home | Food | Drugs | Medical Devices | Radiation-Emitting Products | Vaccines, Blood & Biologics | Animal & Veterinary | Cosmetics | Tobacco Products

### Establishment Registration & Device Listing

FDA Home | Medical Devices | Databases

1 to 2 of 2 Results for **Owner Operator Name :**  
Guangzhou kangling

Results per Page: 10 (dropdown) | New Search

Establishment Name	Registration Number	Current Registration Yr
<a href="#">GUANGZHOU KANGLING BIOTECHNOLOGY CO., LTD</a> CHINA	No number listed	2022
• <a href="#">Non-Surgical Isolation Gown - Kangling</a>		Manufacturer
• <a href="#">Latex Patient Examination Glove - Kangling</a>		Contract Manufacturer; Manufacturer
• <a href="#">Polymer Patient Examination Glove - Kangling</a>		Contract Manufacturer; Manufacturer
<a href="#">GUANGZHOU KANGLING MEDICAL SUPPLIES COMPANY LIMITED</a> CHINA	3017125486	2021
• <a href="#">N95 Respirator With Antimicrobial/Antiviral Agent For Use By The General Public In Public Health Medical Emergencies</a>		Manufacturer
• <a href="#">Face Mask Per Enforcement Policy For Face Masks And Respirators During The Declared Public Health Emergency</a>		Manufacturer

Can't find what you're looking for? [Try a new search](#)

Page Last Updated: 01/10/2022  
Note: If you need help accessing information in different file formats, see Instructions for Downloading Viewers and Players.  
Language Assistance Available: Español | 繁體中文 | Tiếng Việt | 한국어 | Tagalog | Русский | العربية | Kreyòl Ayisyen | Français | Polski | Português | Italiano | Deutsch | 日本語 | فارسی | English

Accessibility | Contact FDA | Careers | FDA Basics | FOIA | No FEAR Act | Nondiscrimination | Website Policies / Privacy

# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## QUALITY CONTROL

- TUV test report

Produkte  
Products



<b>Prüfbericht-Nr.:</b> Test Report No.:	<b>60372571 001</b>	<b>Auftrags-Nr.:</b> Order No.:	<b>168262240</b>	Seite 1 von 12 Page 1 of 12
<b>Kunden-Referenz-Nr.:</b> Client Reference No.:	N/A	<b>Auftragsdatum:</b> Order date:	Apr. 24, 2020	
<b>Auftraggeber:</b> Client:	<b>GuangZhou KangLing Medical Supplies Limited</b> Room 802, Building 1, MingZhu Avenue South No.30, Mingzhu industrial Park, Conghua District, Guangzhou, Guangdong, 510900, P.R. China			
<b>Prüfgegenstand:</b> Test item:	Disposable Medical Face Masks			
<b>Bezeichnung / Typ-Nr.:</b> Identification / Type No.:	Flat Type/Earloop style: 17.5cm x 9.5cm 3ply			
<b>Auftrags-Inhalt:</b> Order content:	Type test			
<b>Prüfgrundlage:</b> Test specification:	EN 14683:2019+AC:2019 except for clause 5.2.6			
<b>Wareneingangdatum:</b> Date of receipt:	Apr. 27, 2020	See Attachment: Photo documentation for details.		
<b>Prüfmuster-Nr.:</b> Test sample No.:	20200414			
<b>Prüfzeitraum:</b> Testing period:	Apr. 28, 2020 to May 15, 2020			
<b>Ort der Prüfung:</b> Place of testing:	See page 3			
<b>Prüflaboratorium:</b> Testing laboratory:	TÜV Rheinland (Shenzhen) Co., Ltd.			
<b>Prüfergebnis:</b> Test result:	Pass			
<b>geprüft von / tested by:</b>	<i>Javen Ke</i>		<b>kontrolliert von / reviewed by:</b>	
Jun. 04, 2020 Javen Ke/Assistant Project Engineer	Jun. 05, 2020 Angela Chen / Department Manager		<i>Angela Chen</i>	
<b>Datum</b> Date	<b>Name / Stellung</b> Name / Position	<b>Unterschrift</b> Signature	<b>Datum</b> Date	<b>Name / Stellung</b> Name / Position
<b>Sonstiges / Other:</b>				
- The test report consists of EN 14683 test report including this cover page (12 pages) and attachment: Photo documentation (6 pages).				
- The Biocompatibility (clause 5.2.6) is not evaluated in this test report.				
<b>Zustand des Prüfgegenstandes bei Anlieferung:</b> Condition of the test item at delivery:		<b>Prüfmuster vollständig und unbeschädigt</b> Test item complete and undamaged		
* Legende: 1 = sehr gut 2 = gut 3 = befriedigend 4 = ausreichend 5 = mangelhaft P(ass) = entspricht o.g. Prüfgrundlage(n) F(ail) = entspricht nicht o.g. Prüfgrundlage(n) N/A = nicht anwendbar NT = nicht getestet				
Legend: 1 = very good 2 = good 3 = satisfactory 4 = sufficient 5 = poor P(ass) = passed a.m. test specification(s) F(ail) = failed a.m. test specification(s) N/A = not applicable NT = not tested				
Dieser Prüfbericht bezieht sich nur auf das o.g. Prüfmuster und darf ohne Genehmigung der Prüfstelle nicht auszuweisweise vervielfältigt werden. Dieser Bericht berechtigt nicht zur Verwendung eines Prüfzeichens. This test report only relates to the a. m. test sample. Without permission of the test center this test report is not permitted to be duplicated in extracts. This test report does not entitle to carry any test mark.				

# CHINA GUANGZHOU KANGLING MEDICAL

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## QUALITY CONTROL

- SGS test report



SGS-P-7.4-01-F02-CRS-SL-EPM

Report No.: CANWT00390839

SGS-CSTC Standards Technical Services Co., Ltd. Guangzhou Branch  
198Kezhu Road, Sdentech Park, Guangzhou Economic & Technology Development District, Guangzhou, Guangdong Province, China  
P.C:510663  
Tel:86 020 82155555  
Fax:86 020 82075008

### INSPECTION REPORT

(Special for Epidemic prevention materials)

**IMPORTANT INFORMATION REGARDING THE SCOPE AND LIMITATIONS OF THE INSPECTION AND REPORT**

The scope of this report is limited to a VISUAL INSPECTION ONLY for the workmanship and basic function check of the product. Performance index and compliance of the product are NOT included in the scope of this report. This report is a reasonable attempt to identify any obvious or significant defects apparent in those areas of the product fully accessible and visible to the inspector at the time of the inspection. This Report is made solely for the use and benefit of the Client named on the front of this report.

**SGS does not verify authenticity of any Brand/Trademark of products. Buyers must check if the product is genuine with the Brand/Trademark owner directly.**

To :	GINMEDICAL DIRECT, LLC	Date:	17-Nov-2021
Attn :	MR. MOSES L. PERRY JR.		
From :	Mandy-WB Huang	E-mail :	mandy-WB.huang@sgs.com

SGS File No.:	CNCAN22250198	Product family view
Buyer :	GINMEDICAL DIRECT, LLC	
Supplier :	GUANGZHOU KANGLING BIOTECHNOLOGY CO., LTD.	
Manufacturer :	GUANGZHOU KANGLING MEDICAL SUPPLIES LIMITED	
Style Number:	KOOLINE	
Product description:	DISPOSABLE PROTECTIVE MASK	
P.O. Number:	21WX/TG001	
L/C Number:	N/A	
Service performed :	FRI	
Inspection Date :	16-Nov-2021	
Inspection Location :	Guangzhou, Guangdong, China	

**Inspection Criteria**

Reference sample provided by	By Manufacturer
Client instruction/specification	Yes
SGS WI number	P-INSP-WI-SL-016
Other	N/A

<b>Overall Inspection Conclusion:</b>	<b>Subject to client's Decision</b>
---------------------------------------	-------------------------------------

**Inspection Summary:**

1. Workmanship appearance :	Conform
2. Quantity :	Conform
3. Style, Material, Colour :	Conform

Inspector: Edward Cai Factory Representative: Crace



Unless otherwise agreed in writing, this document is issued by the Company under its General Conditions of Service available at <http://www.sgs.com/en/Terms-and-Conditions>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein.

Any holder of this document is advised that information contained herein reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law.

Attention: To check the authenticity of issuing inspection report & certificate, please contact us at telephone: 86-755-8327-1942, or email: [CN\\_SCS@sgs.com](mailto:CN_SCS@sgs.com)

SGS (China) Standards Technical Services Co., Ltd. (Guangzhou Branch) Tel: 86-20-8215-5500 136-20-6207-0008 www.sgs.com.cn  
中国 - 广东 - 广州市经济技术开发区科学城萝岗路10号 邮编: 510663 136-20-8215-5555 136-20-6207-5008 sgs.china@sgs.com

[Rev 02: Feb.29th.2021]

Member of the SGS Group (SGS SA)

Page 1 of 21



# CHINA GUANGZHOU KANGLING MEDICAL

---

TAKE RESPONSIBILITY FOR EVERY HEALTHY BREATH

## GUANGZHOU KANGLING BIOTECHNOLOGY CO., LTD

CHINESE MANUFACTURERS: GUANGZHOU KANGLING MEDICAL SUPPLIES CO., LTD.

MANUFACTURER'S ADDRESS: ROOM 802, BUILDING 1, NO. 30, MINGZHU AVENUE SOUTH,  
MINGZHU INDUSTRIAL PARK, CONGHUA DISTRICT, GUANGZHOU CHINA

WEBSITE: [WWW.KANGLINGYIYAO.COM.CN](http://WWW.KANGLINGYIYAO.COM.CN)